


Deep Conical (DC) 03.5mm Parallel Walled Implants - Drill Sequence


Ø3.5mm Parallel Walled (DCC35)




Soft Bone

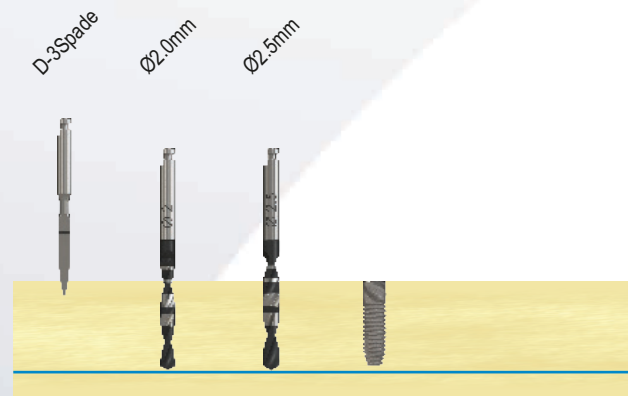

Medium Bone

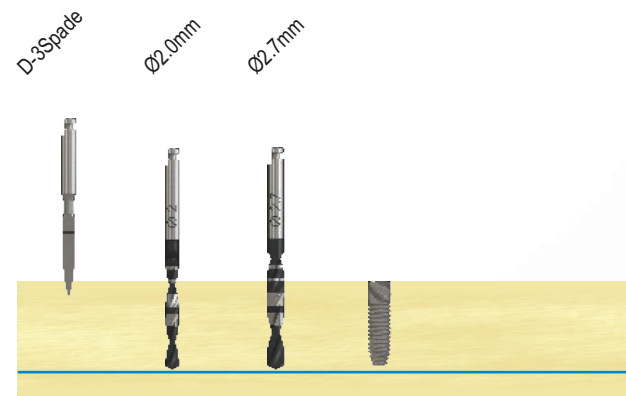

Dense Bone

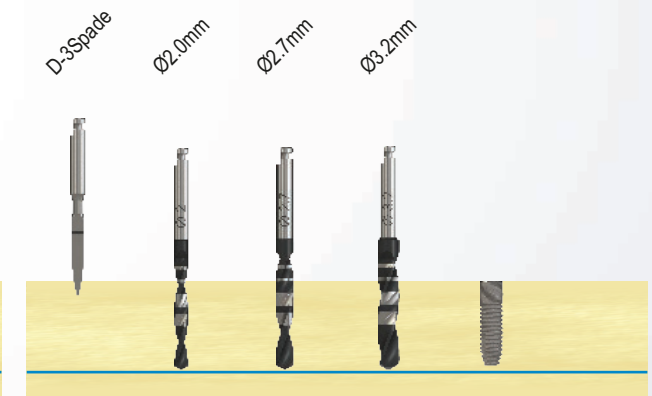

NOTE: Site preparation Sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.