


Deep Conical (DC) 03.5mm Tapered Implants - Drill Sequence


Ø3.5mm Tapered (DCT35)




Soft Bone

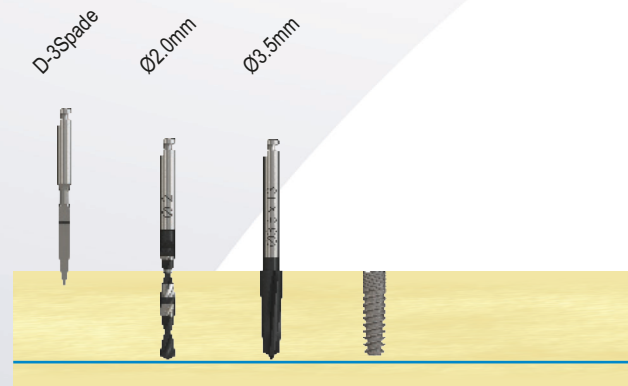

Medium Bone

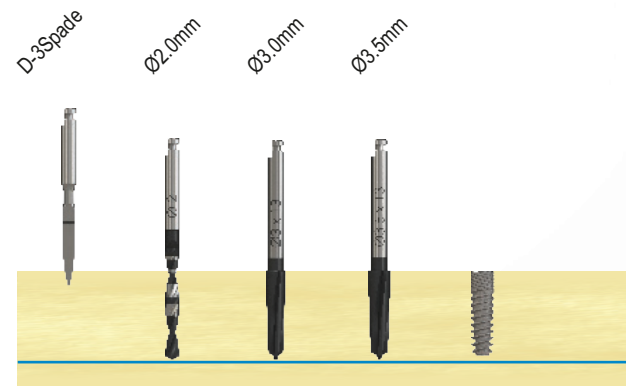

Dense Bone

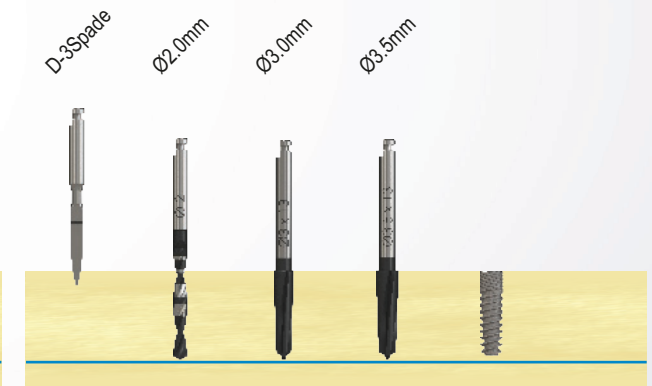

NOTE: Site preparation Sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.



SOUTHERNIMPLANTS

Innovative Treatment Solutions

www.southernimplants.com