



Deep Conical (DC) 05.0mm Tapered Implants - Drill Sequence

Ø5.0mm Tapered (DCT50)


Soft Bone

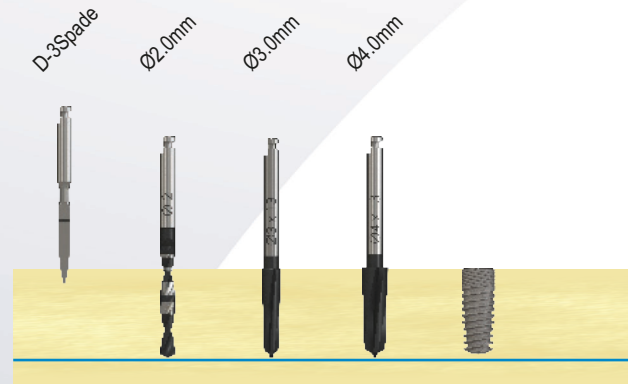

Medium Bone

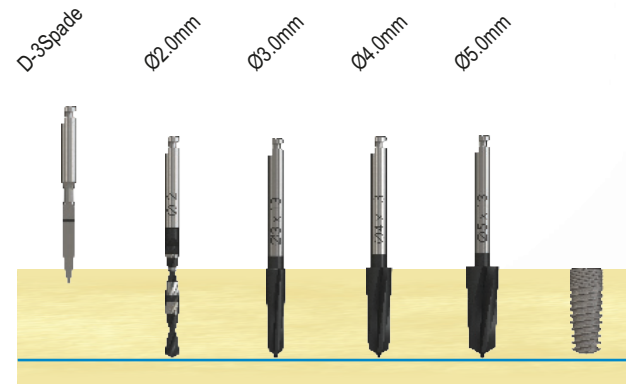

Dense Bone

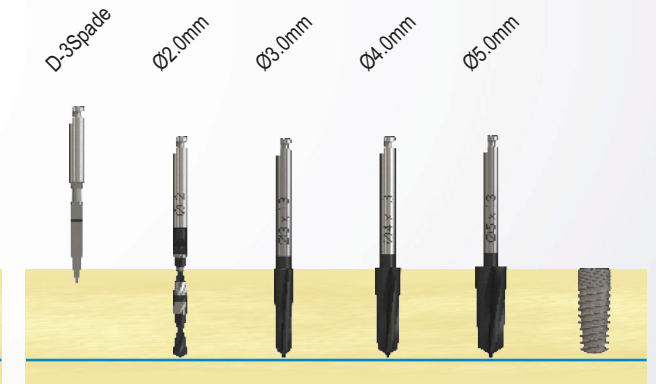

(illustration is for 13mm implants)

NOTE: Site preparation Sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.