


# Deep Conical (DC) 03.5mm Tapered Co-Axis® 12d Implants - Drill Sequence


## Ø3.5mm Tapered (*DCT35-12d Co-Axis*)




### Soft Bone

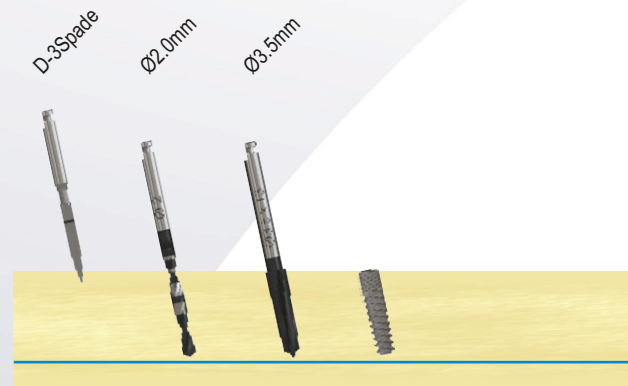

### Medium Bone

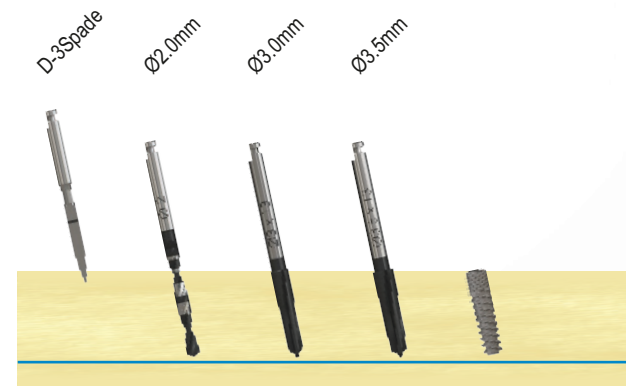

### Dense Bone

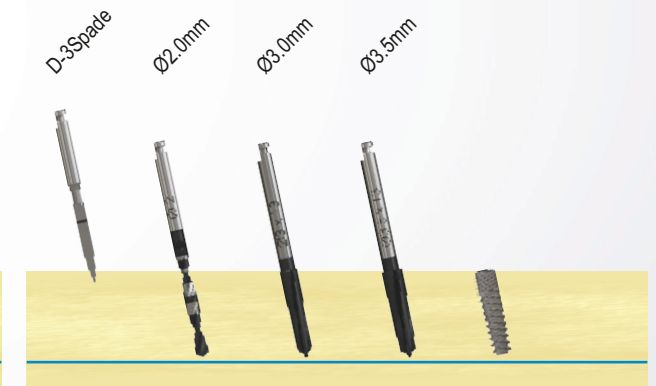

NOTE: Site preparation Sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.



**SOUTHERNIMPLANTS**

Innovative Treatment Solutions

[www.southernimplants.com](http://www.southernimplants.com)