


Deep Conical (DC) 04.0mm Tapered Co-Axis® 12d Implants - Drill Sequence


Ø4.0mm Tapered (DCT40-12d Co-Axis)




Soft Bone

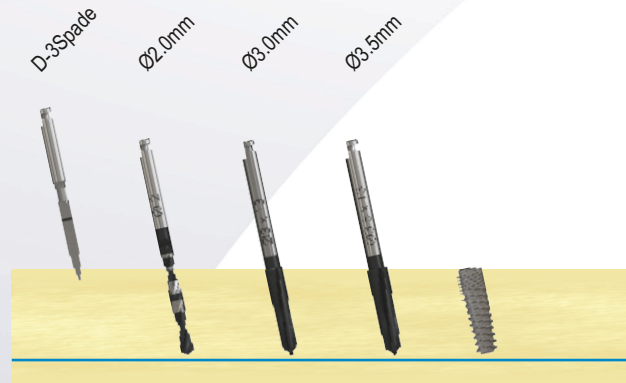

Medium Bone

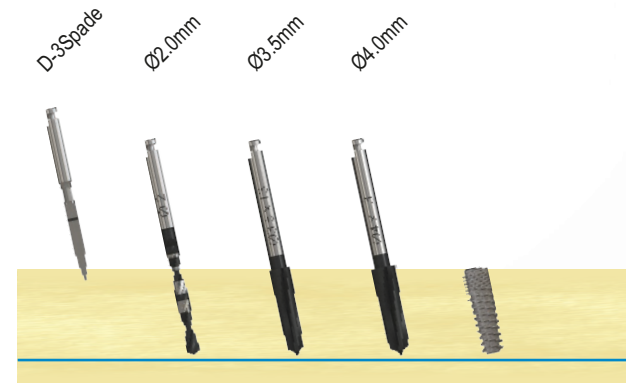

Dense Bone

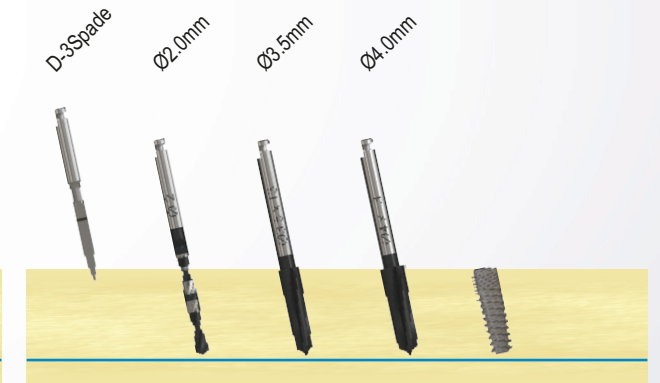

(illustration is for 13mm implants)

NOTE: Site preparation Sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.



SOUTHERNIMPLANTS

Innovative Treatment Solutions

www.southernimplants.com