



External Hex 04.0mm 12° Co-Axis® Implants - Drill Sequence

Tapered (IBT12d / MSc-IBT12d Co-Axis)


Soft Bone

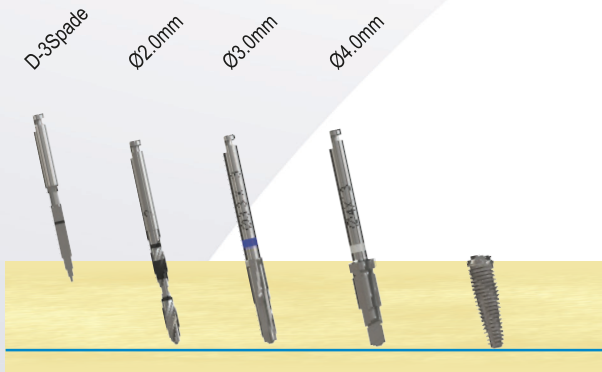

Medium Bone

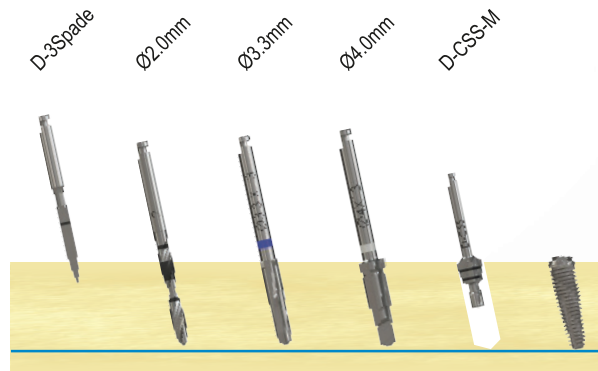

Dense Bone

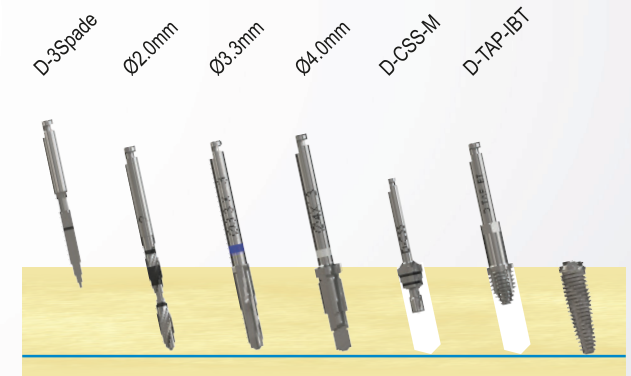

NOTE: Site preparation Sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.
(Illustration is for 13mm implants)