



# External Hex 06.0mm MAX Implants (Tapered) - Drill Sequence

## Tapered (MAX-6 / MSc-MAX-6)


### Soft Bone

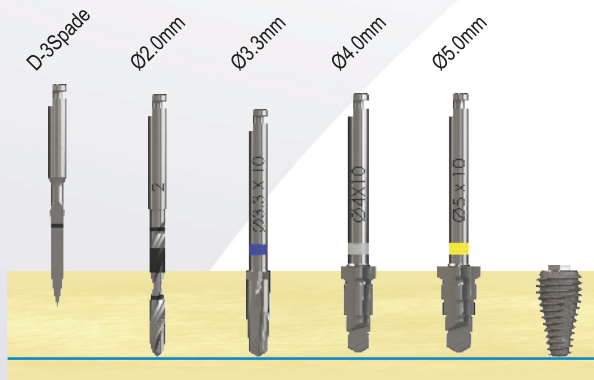

### Medium Bone

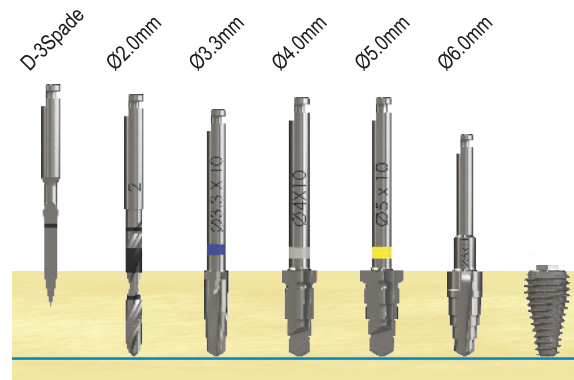

### Dense Bone

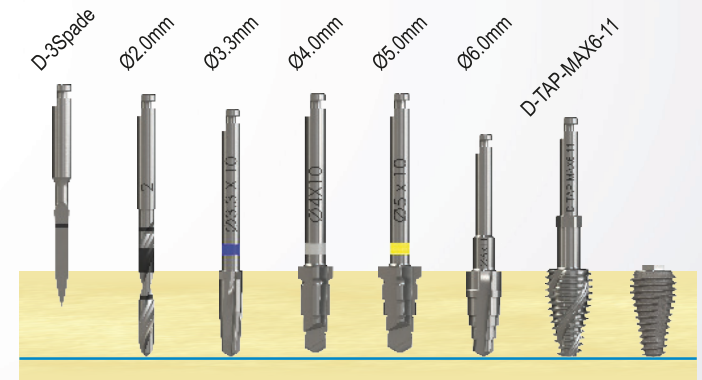

NOTE: Site preparation Sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.  
(Illustration is for 13mm implants)