


Deep Conical (DC) 04.0mm Tapered Implants - Drill Sequence


Ø4.0mm Tapered (DCT40)




Soft Bone

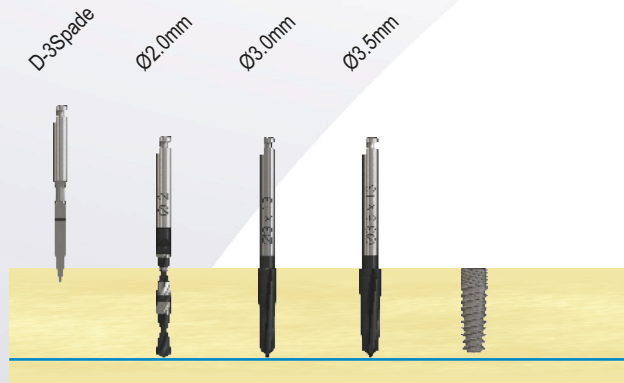

Medium Bone

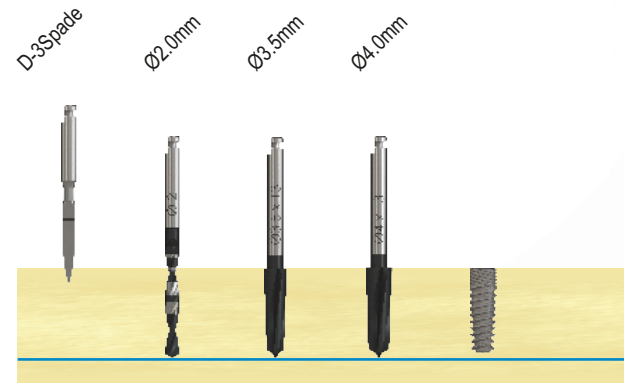

Dense Bone

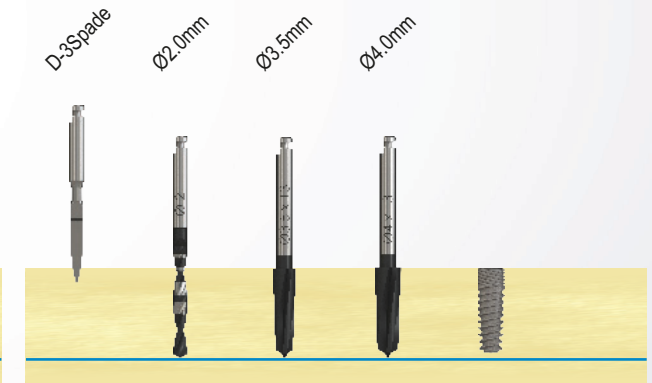

NOTE: Site preparation Sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.