

INTERNAL HEX Implants
Product Catalogue





Southern Implants is a leading provider of unique and innovative dental implant products with a focus on top-end professional users who want more choices. Southern's expertise in research, development and manufacturing of dental implants allows us to provide Innovative Treatment Solutions that will reduce treatment times and improve patient outcomes.

Striving for excellence and meeting customer needs, has led to our wide product range characterized by Unique and Innovative products which include;

- Multiple interfaces, to suit customer preference.
- INVERTA™ implant, featuring a body-shift design, engineered for primary stability and suitable for immediate loadina.
- Co-Axis®, sub-crestal angle correcting implant, available in angulations of 12, 24 & 36° and various internal and external connections.
- MAX implant, specifically designed for immediate molar tooth replacement.
- The ZYGAN and ZYGEX implants for severely resorbed maxilla and craniofacial reconstruction.

Our product portfolio is in synchronized evolution with protocol improvements and technological advances.

 $My \, since re\, thanks\, to\, all\, specialists, dentists\, and\, technicians\, who\, put\, their\, trust\, in\, our\, company.$ 

Graham Blackbeard Managing Director, Southern Implants

### CONTENTS

Ø3.75mm / Ø4.2mm / Ø5.0mm Implants (Tapered) Implants & Surgical Components Prosthetic Flowchart Site Preparation & Instrumentation	Page 06 Page 07 Page 08
CO-AXIS®  Ø4.2mm Co-Axis Implants (Tapered) Implants & Surgical Components. Prosthetic Flowchart. Site Preparation & Instrumentation.	Page 10 Page 11 Page 12
Platform Matched Prosthetics for Ø5mm implants Prosthetic Flowchart	Page 14 Page 15
Insertion Tool Depth Markings	Page 15
Drill Information.	Page 16
Insertion Tool Protocol Implant Placement Procedure for Straight Internal Hex implants	Page 16
Co-Axis® Fixture Mount Removal Protocol	Page 16
Driver Information	Page 17
Instrument Trays I-INT-HEX-EG	Page 18 Page 20
Torque Table for Southern Screws	Page 21
Implant Information	Page 22
Explanation of Symbols	Page 23

NOTE: • Images are for illustration purposes only and do not necessarily accurately represent the product.

- All dimensions in this catalogue are in mm, unless otherwise specified.
- Not all products are cleared for sale in all countries.

# **INTERNAL HEX**

Ø3.75mm / Ø4.2mm / Ø5.0mm







**IM-T50** 

### Implants are available in lengths of:

ITEM CODE TAPERED	IMPLANT LENGTHS (in mm)
IM-T3708	8.0
IM-T3710	10.0
IM-T3711	11.5
IM-T3713	13.0
IM-T3715	15.0

ITEM CODE TAPERED	IMPLANT LENGTHS (in mm)
IM-T4208	8.0
IM-T4210	10.0
IM-T4211	11.5
IM-T4213	13.0
IM-T4215	15.0
IM-T4218	18.0


ITEM CODE TAPERED	IMPLANT LENGTHS (in mm)
IM-T5008	8.0
IM-T5010	10.0
IM-T5011	11.5
IM-T5013	13.0
IM-T5015	15.0

NOTE: Implant dimensions and information - page 22

# **Surgical Components**


# Cover Screw Healing Abutments CS-M HA-M-37 HA-M-45 HA-M-55 Ø3.7 Ø3.7 Ø4.5 Ø4.5 Ø4.5 Ø3.6 Ø3.7 Ø4.6 lengths 3/4/6 lengths

### **Prosthetic Flowchart**

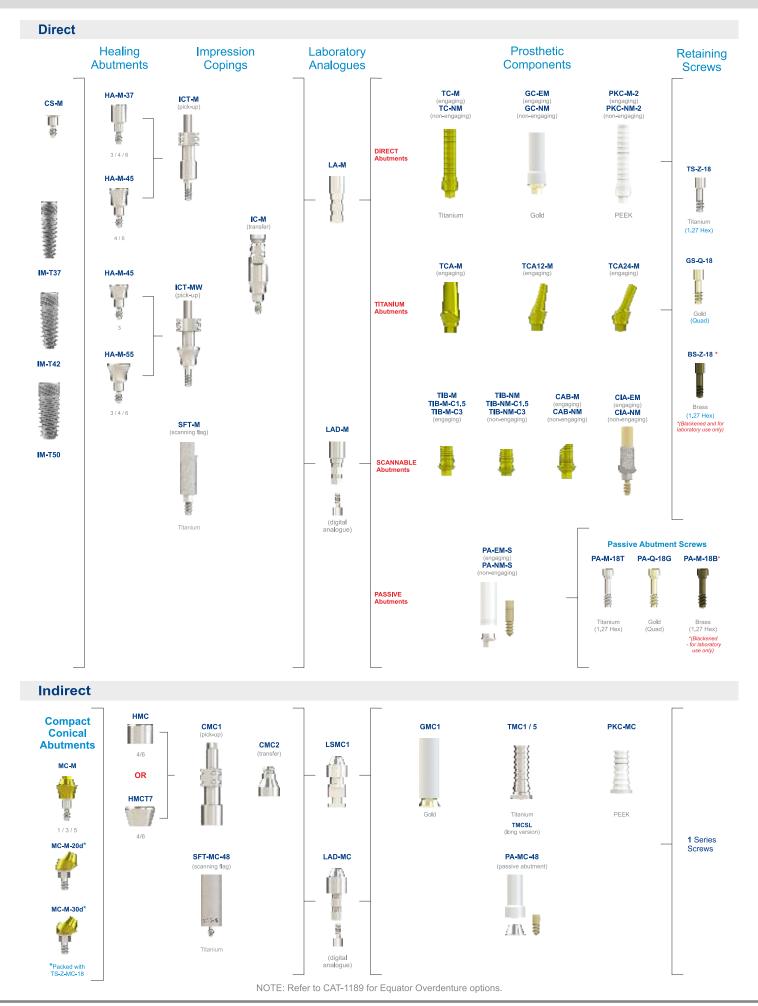


# **Site Preparation Sequence**


### Ø3.7mm Tapered (IM-T37)

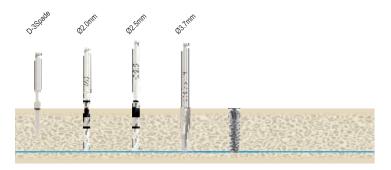

### Ø4.2mm Tapered (IM-T42)

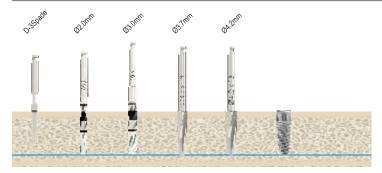

### Ø5.0mm Tapered (IM-T50)

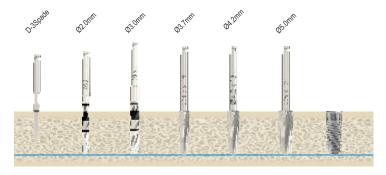

(All illustrations are for 13mm implants)

- NOTE: Site preparation sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.
  - Refer to page 16 for the Fixture Mount Removal Protocol.

### Instrumentation



- NOTE: Refer to CAT-1155 for more information on wrench insert converters
  - Most instruments are available in various lengths

# INTERNAL HEX CO-AXIS®

Ø4.2mm



IM-T42-12d

# Implants are pre-mounted and available in lengths of:


NOTE: Implant dimensions and information - page 22

ITEM CODE	IMPLANT LENG	THS (in mm)
TAPERED	L1	L2
IM-T4208-12d	8.0	8.3
IM-T4210-12d	10.0	10.3
IM-T4211-12d	11.5	12.3
IM-T4213-12d	13.0	13.3
IM-T4215-12d	15.0	15.3
IM-T4218-12d	18.0	18.3

# **Surgical Components**


Cover Screw	Healing Abuti	ments	
CS-M	HA-M-37	HA-M-45	HA-M-55
	Ø3.7	Ø4.5	Ø5.5
	3/4/6 lengths	3/4/6 lengths	3/4/6 lengths

### **Prosthetic Flowchart**

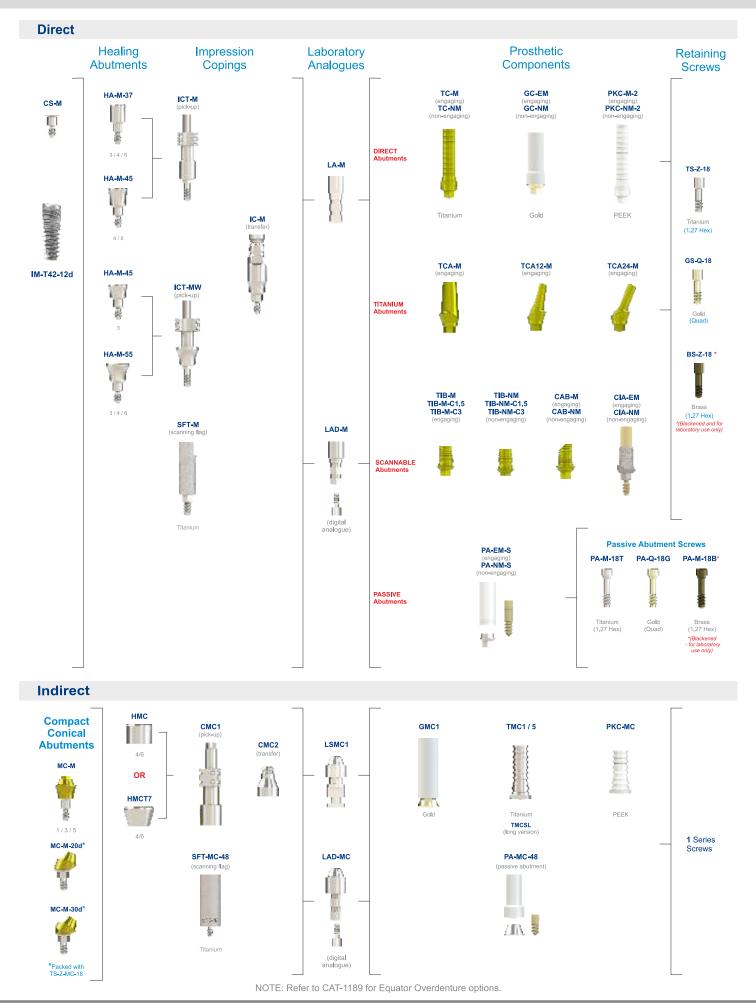

# **Site Preparation Sequence**

## Ø4.2mm Tapered Co-Axis® (IM-T42-12d)

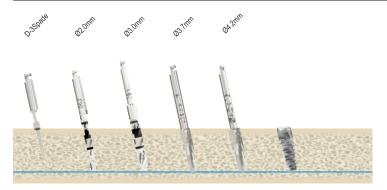

(illustration is for 13mm implants)

NOTE: • Site preparation sequence recommended by Southern Implants does not replace the judgement and experience of the surgeon.


1.22 Universal Hex Driver

Quad Driver

• Refer to page 16 for the Fixture Mount Removal Protocol.

### Instrumentation



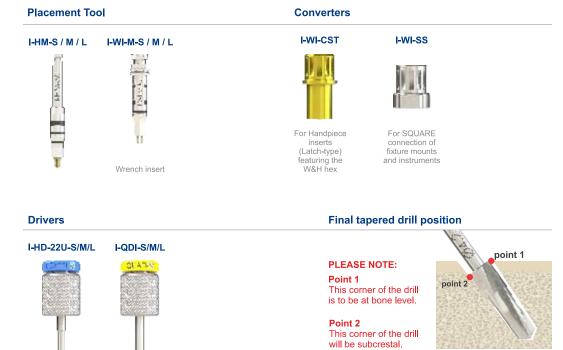

NOTE: • Refer to CAT-1155 for more information on wrench insert converters • Most instruments are available in various lengths

# **PLATFORM MATCHED PROSTHETICS**

for Ø5mm implants


### PLATFORM MATCHED PROSTHETICS for Ø5mm implants

In applications of the Internal Hex Ø5mm implants, for single posterior teeth, where the patient is known to have a very strong bite force, the clinician may choose to follow this "Platform Matched" approach. This approach uses the implant platform, in order to give the single tooth prosthetics greater stability.


**Warning**: These Platform Matched Prosthetics are not compatible with Internal Hex Ø3.7mm/ Ø4.2mm implants or Internal Hex Co-Axis<sup>™</sup> Ø4.2mm implants.



Implants with Standard Interface



Standard internal cone interfacing prosthetics



Platform Matched Prosthetics

### Compatible with:


NOTE: Implant dimensions and information - page 22

ITEM CODE TAPERED	IMPLANT LENGTHS (in mm)
IM-T5008	8.0
IM-T5010	10.0
IM-T5011	11.5
IM-T5013	13.0
IM-T5015	15.0


### **Surgical Components**

Cover Screw	Healing Abutments	
CS-M	HA-M-P45	
	Ø4.5	
	3/4/6 lengths	

### **Prosthetic Flowchart**

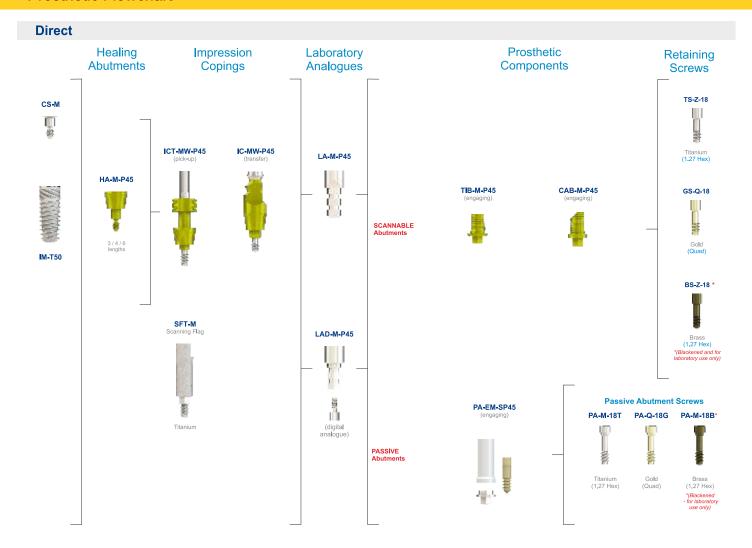

### INSERTION TOOL DEPTH MARKINGS

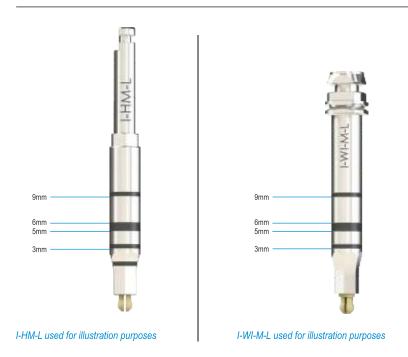


NOTE:  $\,\,\bullet\,\,$  Laser markings at 3mm, 5mm, 6mm and 9mm from implant platform.

• Refer to CAT-1201 for Insertion Tool markings and depths.

Important: The PEEK bits (I-PBIT-L18) should be replaced on a regular basis. General wear & tear are to be expected with regular use. Items sold separately.

### **Twist Drill Markings**





### INSERTION TOOL PROTOCOL

### Implant Placement Procedure for Straight Internal Hex implants

- 1. The tool I-HM-S/M/L is used to pick up the implant from the packaging.
- 2. The hexagon of the insertion tool in the implant must be fully engaged before torque is applied, to prevent any damage [The hexagon is fully engaged when the straight portion of the hexagon tool is almost completely sunken in the implant (fig. 1)].
- 3. The implant is placed in the prepared site and screwed in with a motor unit at 15rpm while applying downwards pressure.



### CO-AXIS<sup>TM</sup> FIXTURE MOUNT REMOVAL PROTOCOL

- 1. The tool I-HM-S / M / L is used to pick up the implant from the packaging (fig 1) using the fixture mount.
- 2. Once the implant is placed, the position verified, and after final X-rays have been taken, remove the fixture mount by unscrewing the fixture mount screw using a I-HD-22U-S/M/L handheld driver (fig 2).





### **Drivers**



### **Abutment Drivers** (for Compact Conical Abutments)





### **Driver Information for 1 Series Screws**



Refer to CAT-1203 for alternative Drivers

I-INT-HEX-EG for surgical placement of Internal Hex Implants

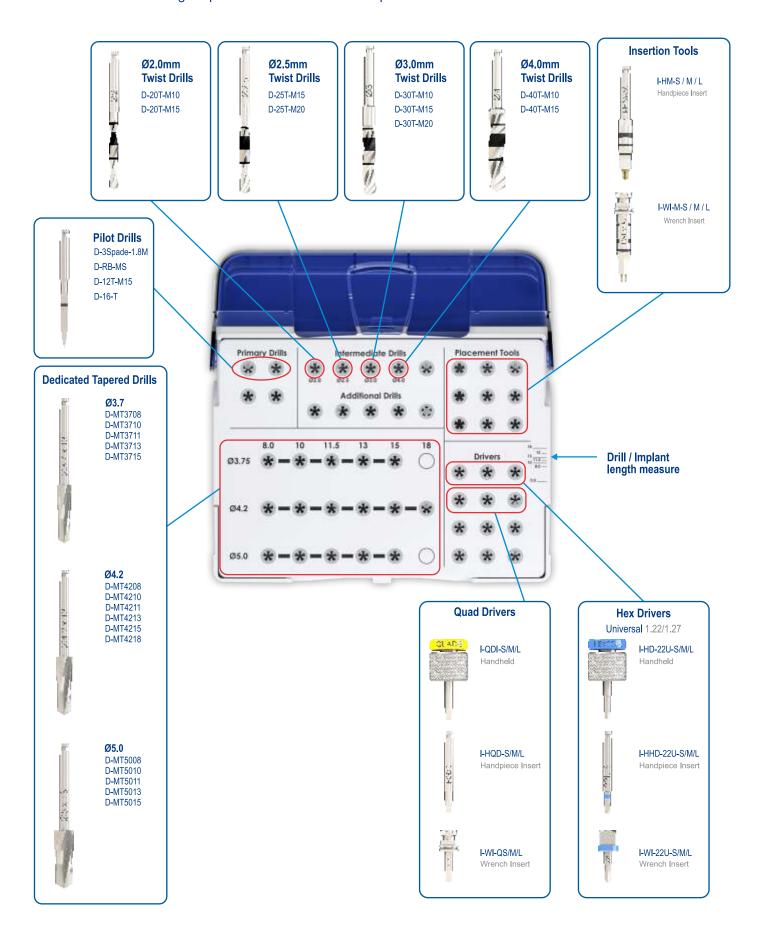


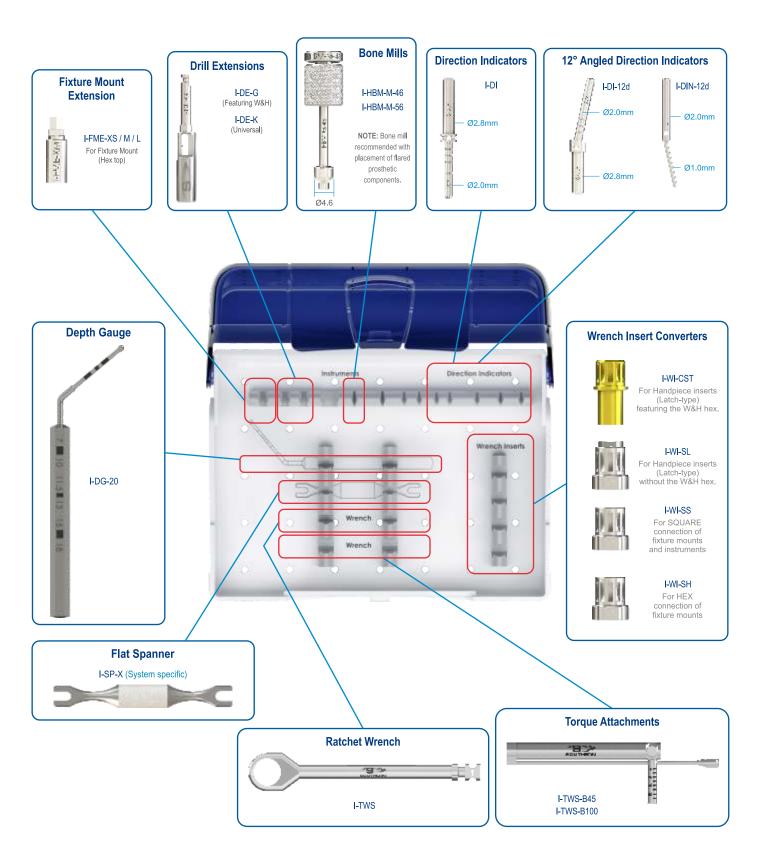

### NOTE:

- The surgical kit has an intuitive layout to guide the surgeon through the drill sequence.
- · Most Instruments available in various lengths.
- All instruments and tooling used during the procedure must be maintained in good condition, and cleaned and sterilized prior to to use. Please consult the Southern Implants Cleaning and Sterilization Procedure Guidelines (CAT-1039) for guidance concerning the maintenance of drills, instruments, and surgical trays.

### I-PROS-EG Prosthetic Instrument Tray

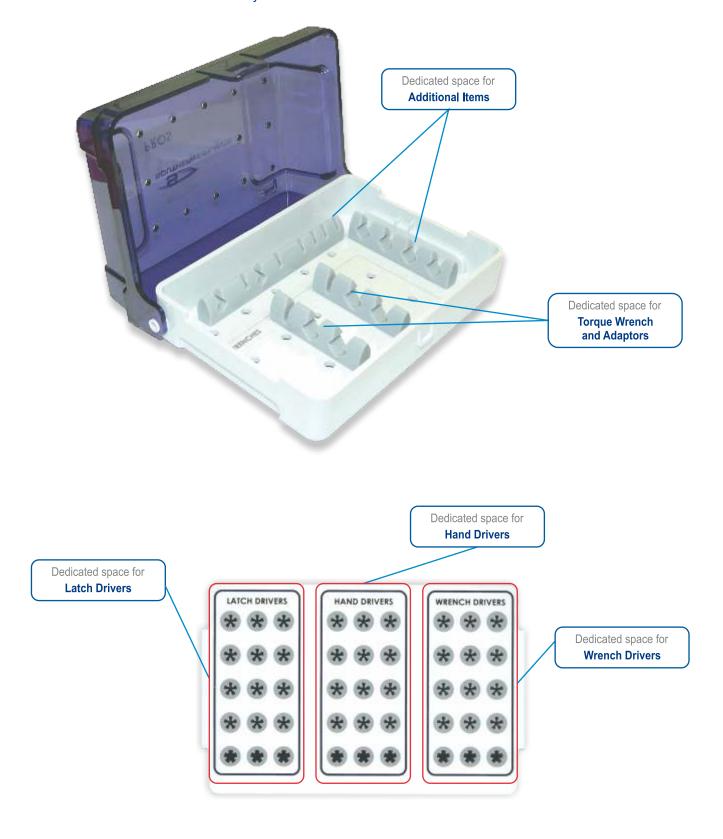

### NOTE:

- This instrument tray is to be *customised by the user* to be suitable for use with the preferred implant system and its surgical or prosthetic items.
- Most Instruments available in various lengths.

### 1.27 Hex Prosthetic screws



### **Quad Prosthetic screws**



TORQUE: 32Ncm Head Diameter: 2.25mm Screw TORQUE with PEEK Prosthetics:

### 1.27 Hex Passive Abutment screws

### **Quad Passive Abutment screws**



PA-M-18T







TORQUE: 32Ncm Head Diameter: 2.60mm

# **Digital Laboratory Analogue screw**

1.22 Hex



LAD-S

TORQUE: Finger tighten Head Diameter: 2.40mm

# **TIB Abutment screw**



TS-IT-TIB

TORQUE: 32-40Ncm **Head Diameter:** 2.40mm

NOTE: Screw supplied with all Digital Analogues

### 1 Series screws

### M1.4



TSH1











Unigrip



1.22 Hex





GSH1



BSH1\*





GSU1

TORQUE: 10-15Ncm Head Diameter: 2.25mm Screw TORQUE with PEEK Prosthetics: 10 - 15Ncm

NOTE:

- Due to design revisions screw tips may be flat or rounded.
- Always ensure that the correct screw is used for the relevant implant and component.
- \* Blackened and for laboratory use only.

### **Screw Head Connections**

Hex








Unigrip




RANGE												MPL	IMPLANT LENGTH CODES	ENG.	гн сс	DES	
		MAJOR DIAMETER		IMPLANT PROSTHETIC PLATFORM DIAMETER DIAMETER	Prosthetics	HEX WIDTH (across flats)	SMOOTH COLLAR HEIGHT	THREAD	APEX DIAMETER	Cylindrical PLATFORM or Tapered ANGLE C/T	PLATFORM ANGLE	<b>∞</b>	10	<b>±</b>	13	15	18
IM-T37	Ø3.75mm	3.83	3.75	3.6	•	2.44	0:30	1.0	3.1	<b>—</b>		>	>	>	>	>	
IM-T42	Ø4.2mm	4.2	3.75	3.6		2.44	0.27	1.0	3.7	<b>-</b>		~	>	>	>	>	>
IM-T50	Ø5.0mm	5.0	4,55	3.6/4.5	/	2.44	0.27	1.0	4.5	<b>—</b>		>	>	>	>	>	
IM-T42-12D	Ø4.2mm	4.2	3.75	3.6		2.44	0.15	1.0	3.7	⊢	12°	^	>	>	~	>	>
All dimensions in this catalogue are in mm, unless otherwise specified.	are in mm, unless	otherwise specifi	ied.														

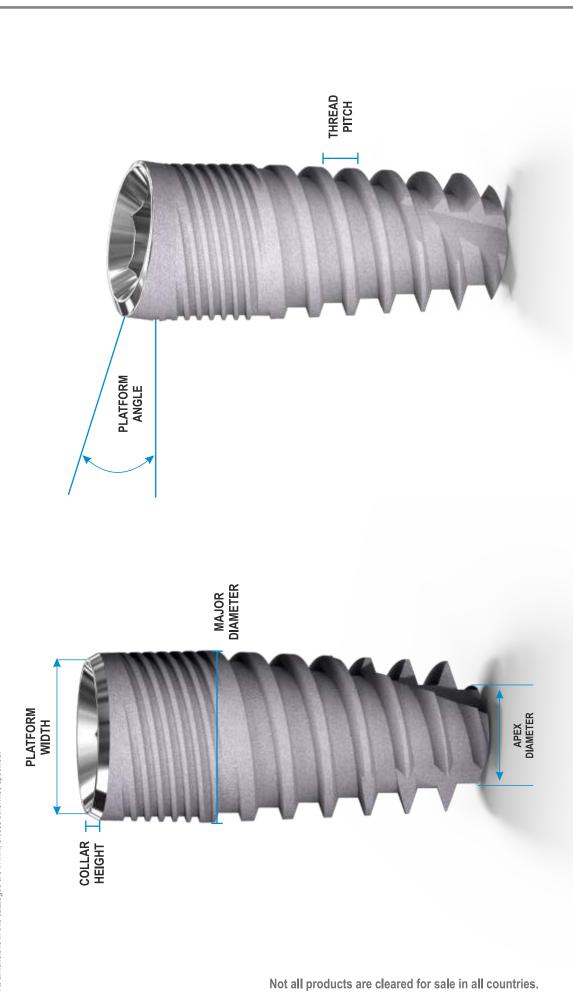

### The following symbols are used on our packaging labels and they indicate the following:

- 1 Manufacturer
- Implant image
- 3 Implant details and size
- 4) STERLER Sterilization using Irradiation
  - Do not Resterilize
  - Consult instruction for use
  - ② Do not reuse
  - **CE** mark and notified body number
  - **Expiry date**
  - Sterile unless package is opened or damaged
- 2D Bar coding Contains the GTIN, Expiry Date and LOT Number
- 6 Patient sticker for documentation purposes (to be used by health care provider on patient file)
- 7 R Prescription device

  CAUTION: FEDERAL LAW RESTRICTS THE DEVICE TO SALE BY OR ON THE ORDER OF A LICENCED HEALTH CARE PROVIDER.







### **Platform Interface**

Ø3.75

Ø4.2

Ø5.0



For more information, please contact your Southern Implants Representative or visit southernimplants.com



**South Africa - Headquarters** 1 Albert Road, Irene, RSA **T:** +27-12-667-1046 | **E:** info@southernimplants.com

### **Subsidiaries**

**Australia**Southern Implants Australia **T:** +61-2-8076-9337

**E:** info@southernimplants.com.au

**United Kingdom** 

Southern Implants UK
T: +44-20-8899-6845 / 6 / 7
E: info@southernimplants.co.uk

**USA** and Canada

Southern Implants North America Inc. T: +1-561-472-0990 E: customercare@southernimplants.com

 $\textbf{Southern Implants Products are distributed world-wide, please visit southern implants.com for a list of \textbf{Distributors.}}$ 

©2019 Southern Implants (Pty) Ltd. All rights reserved. Co-Axis, Southern Implants, and Subcrestal Angle Correctionare registered trademarks and Body-Shift, INVERTA and PROVATA are trademarks of Southern Implants (Pty) Ltd. Not all implants are available in all markets.