

English	INSTRUCTIONS FOR USE: Southern Implants® Internal Octagon (IT) Implants
Español	INSTRUCCIONES DE USO: Southern Implants® Internal Octagon (IT) Implants
Italiano	ISTRUZIONI PER L'USO: Southern Implants® Internal Octagon (IT) Implants
Français	MODE D'EMPLOI : Southern Implants® Internal Octagon (IT) Implants
Deutsch	GEBRAUCHSANWEISUNG: Southern Implants® Internal Octagon (IT) Implants
Português	INSTRUÇÕES DE UTILIZAÇÃO: Southern Implants® Internal Octagon (IT) Implants

ARCHIVED



South Africa - Headquarters 1 Albert Road, Irene, RSA
T: +27-12-667-1046 | **E:** info@southernimplants.com

Subsidiaries

Australia

Southern Implants Australia
T: +61-2-8076-9337
E: info@southernimplants.com.au

Spain and Portugal

Southern Implants Ibérica
T: +34 935 053 507
E: info@southernimplants.es

EC REP

United Kingdom and Ireland

Southern Implants UK
T: +44-20-8899-6845 / 6 / 7
E: info@southernimplants.co.uk

USA and Canada

Southern Implants North America Inc.
T: +1-561-472-099
E: customercare@southernimplants.com

Intended use

The devices are intended to treat partially or fully edentulous patients eligible for placement of one or more dental implants as a means of fixing a permanent or removable single crown, partial or full-arch dental prosthesis in the upper or lower jaw. The devices allow for immediate or delayed prosthetic restoration based on the user's evaluation of the patient's eligibility.

Intended user

Maxillo-facial Surgeons, General Dentists, Orthodontists, Periodontist, Prosthodontists and other appropriately trained and experienced implant users.

Intended environment

The implants are intended to be used in a clinical environment such as an operating theater or a dentist consultation room.

Intended patient population

This device is used in the dental restoration of partially or fully edentulous patients in the upper or lower jaw. Restorations may comprise single teeth, partial or full bridges, and may be fixed or removable.

Description


The Internal Octagon implant is a self-tapping implant made of commercially pure special Grade 4 titanium. Implants are available with either a tapered or parallel walled body shape. All implants are surface-roughened up to the collar using Southern Implants' proven surface. The surface has a S_a value of 1.4 microns. The Internal Octagon implant is also available in the angulated platform Co-Axis® design, with a built-in platform angulation of 12°, this design enables tilting of the implant without compromising the restorative emergence angle. Implants packed with a fixture mount is also supplied with a cover screw in the base of the packaging tube (*Illustration 1*). Cover screws and healing abutments are sold separately for range without fixture mount.

TABLE A

IT (Internal Octagon)				Straight Implants
	CODE	LENGTHS	LENGTHS *	
Ø3.3	ITC3	6 / 8 / 10 / 12 / 14	6f / 8f / 10f / 12f / 14f	Cylindrical
Ø4.0	ITT4	8 / 10 / 12 / 14	8f / 10f / 12f / 14f	Tapered
Ø4.1	ITC4	6 / 8 / 10 / 12 / 14	6f / 8f / 10f / 12f / 14f	Cylindrical
Ø4.9	ITC5	6 / 8 / 10 / 12 / 14	6f / 8f / 10f / 12f / 14f	Cylindrical
Ø4.9*	ITC6-5	6 / 8 / 10 / 12 / 14	6f / 8f / 10f / 12f / 14f	Cylindrical
Ø5.0	ITT5	8 / 10 / 12 / 14	8f / 10f / 12f / 14f	Tapered
Ø5.0*	ITT6-5	8 / 10 / 12 / 14	8f / 10f / 12f / 14f	Tapered
Ø6.0*	ITT6	8 / 10 / 12 / 14	8f / 10f / 12f / 14f	Tapered

* Implants with (f) in code indicates with fixture mount & packed with cover screw


* Wide Interface



IT (Internal Octagon)			Co-Axis®
	CODE	LENGTHS	
Ø4.0	ITST12d-4xxf	8 / 10 / 12 / 14	Tapered
Ø5.0	ITST12d-5xxf	8 / 10 / 12 / 14	Tapered

Prosthetic platform angled at 12°

Supplied with fixture mount.

**Indications for use**

Southern Implants Dental Implants are intended for both one- and two-stage surgical procedures in the following situations and with the following clinical protocols:

- replacing single and multiple missing teeth in the mandible and maxilla,
- placement in extraction sites and in situations with a partially or completely healed alveolar ridge,
- especially indicated for use in soft bone applications where implants with other implant surface treatments may be less effective,
- immediate loading in all indications, except in soft bone (type IV) where implant stability may be difficult to obtain and immediate loading may not be appropriate.

Contraindications

Do not use in patients:

- Who are medically unfit for dental implant procedures.
- Where adequate numbers of implants could not be placed to achieve full functional support of the prosthesis.
- Who are allergic or have hypersensitivity to pure titanium or titanium alloy (Ti-6Al-4V), gold, palladium, platinum or iridium.
- Who are under the age of 18, have poor bone quality, blood disorders, infected implant site, vascular impairment, uncontrolled diabetes, drug or alcohol abuse, chronic high dose steroid therapy, anti-coagulant therapy, metabolic bone disease, radiotherapy treatment.

Warnings

THESE INSTRUCTIONS ARE NOT INTENDED AS A SUBSTITUTE FOR ADEQUATE TRAINING

- For the safe and effective use of dental implants, it is suggested that specialised training be undertaken, including hands-on training to learn proper technique, biomechanical requirements and radiographic evaluations.
- Responsibility for proper patient selection, adequate training, experience in the placement of implants, and providing appropriate information for informed consent rests with the practitioner. Improper technique can result in implant failure, damage to nerves/vessels and/or loss of supporting bone.
- For short implants, clinicians should closely monitor patients for any of the following conditions: peri implant bone loss, changes to implant's response to percussion, or radiographic changes in bone to implant contact along the implant's length. If the implant shows mobility or greater than 50% bone loss, the implant should be evaluated for possible removal. If the clinicians choose a short implant, then clinicians should consider a two-stage surgical approach, splinting a short implant to an additional implant, and placement of the widest possible fixture. Allow longer periods for osseointegration and avoid immediate loading.

Cautions

New and experienced Implant users should do training before using a new system or attempt to do a new treatment method. Take special care when treating patients who have local or systemic factors that could affect the healing of the bone and soft tissue. (i.e. poor oral hygiene, uncontrolled diabetes, are on steroid therapy, smokers, infection in the nearby bone and patients who had orofacial radiotherapy.)

Thorough screening of prospective implant candidates must be performed including:

- A comprehensive medical and dental history.
- Visual and radiological inspection to determine adequate bone dimensions, anatomical landmarks, occlusal conditions and periodontal health.
- Bruxism and unfavourable jaw relations must be taken into account.
- Proper pre-operative planning with a good team approach between well trained surgeons, restorative dentists and lab technicians is essential for successful implant treatment.
- Minimising the trauma to the host tissue increases the potential for successful osseointegration.
- Electro-surgery should not be attempted around metal implants, as they are conductive.

Pre-operative examination and planning

A full medical and dental history must be taken, with emphasis on the presence of soft and or hard tissue pathology. The patient must have clinically symptom-free sinuses and no pathology in surrounding bone or soft tissue.

It is recommended that a CT scan and or CBCT analysis be performed as part of the planning process in order to;

- Detect the presence of any pathology in the maxillary sinuses.
- Bone volume and condition.
- Jaw relationships.

- Choose an appropriate size implant for the amount of bone available, without violating the biological width, and evaluate sufficient bone volume surrounding the implant body. In dense bone, use new drills and profuse irrigation. In low-density bone, it is recommended to undersize the osteotomy by drilling with a smaller final drill (i.e. If placing a diameter 5.0mm implant, final shaping drill would be 4.0mm.

Storage, cleaning & sterilisation

The implants, cover screws and healing abutments are supplied sterile (sterilised by gamma irradiation) and intended for single-use prior to the expiration date (see packaging label). Sterility is assured unless the container or seal is damaged or opened. If packaging is damaged do not use the product and contact your Southern representative, or return to Southern Implants.

Do not reuse implants, cover screws, temporary abutments and abutments. Reusing these components may result in:

- Damage on the surface or critical dimensions, which may result in performance and compatibility degradation.
- Adds the risk of cross-patient infection and contamination if single use items are reused.

Southern Implants does not accept any responsibility for complications associated with reused components.

Packaging & Precautions to maintain the sterility of the implant

Implants are packaged as follows:

- An outer package consisting of a rigid, clear box which acts as protection for the inner package.
- The inner package consisting of a blister pack (clear plastic-formed bubble-type base with a TYVEK "peel-back" lid).
- Within the inner package there is a hollow tube which contains one implant suspended from a titanium ring, this ensures the implant never touches the inside of the plastic tube.
- Labelling information is located on the surface of the peel-back lid and on the outside of the rigid box.


Care must be taken to maintain the sterility of the implant by proper opening of the packaging and handling of the implant.

- Open the implant package in the non-sterile field, with non-sterile gloves, tear the address label to open the box.
- With non-sterile gloves remove the inner blister pack. Do not place the plastic box or blister pack-lid onto the sterile field. The contents of this inner package are sterile.
- The sealed blister is to be opened by an assistant (with non-sterile gloves), remove the TYVEK lid and drop or place the sterile tube onto the sterile field, open the tube cap and attach the implant placement tool onto the implant and carefully remove from the sterile tube. Do not touch the sterile implant.

Other sterile components are packed in a peel pouch or blister base with a peel-back lid. Labelling information is located on the bottom half of the pouch, inside the packet or on the surface of the peel-back lid. Sterility is assured unless the pouch is damaged or opened.

Non-sterile components are supplied clean but not sterile in a peel pouch blister base with peel-back lid. Labelling information is located on the bottom half of the pouch, or on the surface of the peel-back lid.

(Illustration 1)

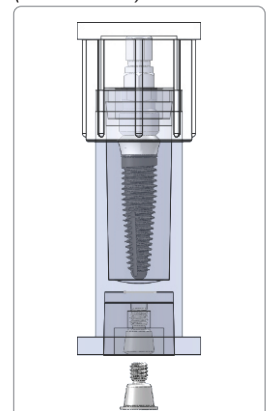

SURGICAL PLACEMENT

PARALLEL WALLED IMPLANTS

Step 1: Initiate the osteotomy (Fig. 1)

Note: It is recommended to raise a full-thickness mucoperiosteal flap.

The 3Spade drill (D-3Spade-1.8M) (Fig. 4A) is used to initiate the osteotomy by perforating the cortical plate at the desired location.

All drilling should be performed at a speed of 1000-1500 rpm with copious irrigation. An intermittent technique should be used to avoid overheating of the bone.


Step 2: Pilot drilling – Ø2.2mm Twist Drill (Fig. 2)

Drill with the Ø2.2mm twist pilot drill (D-220C) (Fig. 4B) to the implant length corresponding to the laser markings on the twist drills and depth gauge (Fig. 4C). **Note:** IT implants are tissue level implants. The implant should be inserted up to the smooth collar.

To verify the alignment with adjacent teeth/implants, insert the direction indicator (I-DI) (Fig. 4D). A radiograph is taken at this point to verify the depth and angulation. If the drilling direction is incorrect, start a new direction with the Ø2mm pilot drill.

Step 3: Gradually enlarge the osteotomy (Fig. 3)

Repeat Step 2 for each consecutive twist drill in the drill sequence corresponding to the selected implant. Drill to the appropriate depth, as indicated by the depth markings on each drill. (Fig. 4E) Insert the direction indicator (I-DI) after using each twist drill.

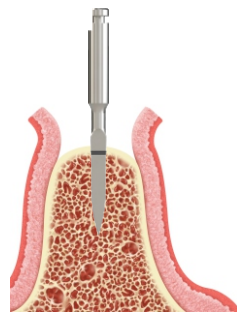

(Fig. 1)




(Fig. 2)



(Fig. 3)

IMPLANT DRILL DEPTH (Fig. 4)

Illustrating placement of a 12 mm implant

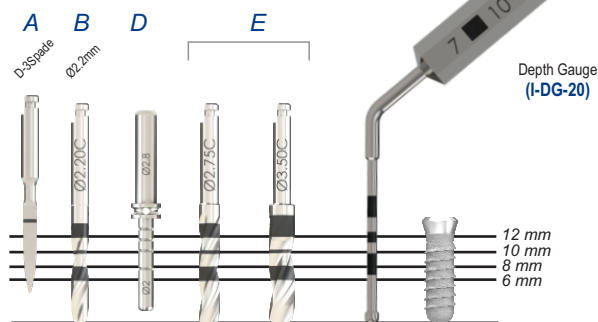

Note

Caution should be taken to not over prepare the implant site, especially for shorter length implants (9mm and shorter).

With a probe, check the soft tissue height, prepare final step at least 1 mm subcrestal. Depending on the gap between planned implant and buccal bone plate, deeper countersinking can be appropriate.

SURGICAL PLACEMENT

TAPERED & CO-AXIS® IMPLANTS

Step 1: Initiate the osteotomy

As per Step 1 (Fig. 1).

Step 2: Pilot drilling – Ø2.2mm Twist Drill As per Step 2 (Fig. 2).

Pilot drilling: Ø2.2mm Twist Drill (Co-Axis® implants)

Drill in the planned angled direction to the appropriate depth, as indicated by the depth markings on the Ø2.2mm twist drill (D-220C). If an anterior implant is being placed, **align the drill to the incisal edge of the adjacent tooth.** (Fig. 5 & 6).

With the 12° Co-Axis® angulation, the screw access hole will come out on the palatal side if aligned correctly.

If the osteotomy is angulated too much to the palatal side (e.g. normal direction when preparing for a screw retained restoration) there is a risk of a sub-optimal restoration angle, with soft and hard tissue being compromised on the palatal side. Insert the direction indicator (I-DI-12d) (Fig. 7).


A radiograph is taken at this point to verify the depth and angulation. If the drilling direction is incorrect, start a new direction with the Ø2mm pilot drill.

Step 3: Gradually enlarge the osteotomy


The Internal Octagon tapered drills are length and diameter specific. Use the length and diameter drill corresponding to the implant that is selected. Widen the osteotomy intermittently to the desired diameter. (Fig. 9E).

Follow the recommended drill protocols for soft, medium and dense bone by referring to catalogue.


Final drill position for Co-Axis® implants. (Fig. 8)

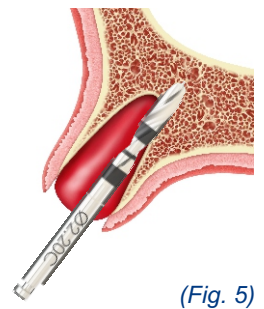


(Fig. 5)

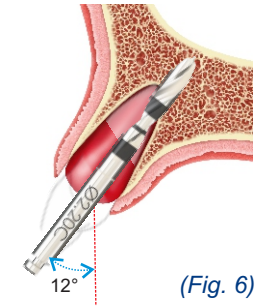

(Fig. 6)

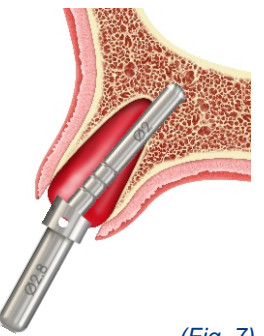

(Fig. 7)



(Fig. 8)

*Final Tapered Drill Position (Co-Axis)


PLEASE NOTE:

Point 1
This corner of the drill is to be at bone level.

Point 2
This corner of the drill will be subcrestal.

IMPLANT DRILL DEPTH (Fig. 9)

Illustrating placement of a 12 mm implant

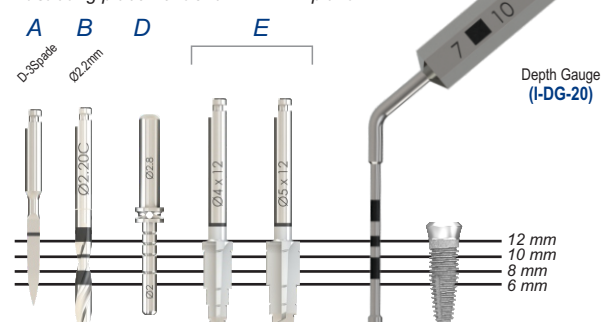

STRAIGHT IMPLANTS (NON-FIXTURE MOUNTED)

Step 4: Implant placement

Surgical procedure for latch insertion tools.

1. Connect the standard insertion tool (I-HITS/-S) to the handpiece of the implant motor unit. (Fig. 10)
2. Engage the octagon of the implant with the insertion tool.
3. Carefully remove the implant from the sterile vial.
4. The insertion tool must be fully engaged in the implant before torque is applied.

NOTE: If the octagon did not align during pick-up then the octagon will engage when implant starts to turn in the bone. The octagon is fully engaged if the top of the octagon is flush with the top of the implant, only then can maximum torque be applied. If they do not engage: change the direction of the rotation, rotate the implant half a turn, change the direction again, this will ensure the engagement of the octagon. (Fig 11 & 12)

Alternatively


1. Connect the standard latch insertion tool (I-HITS/-S) and the wrench converter (I-WI-CST), and insert it into the surgical wrench (I-TWS-B45 /B100).
2. Connect the wrench insertion tool (I-WI-ITS / S) and wrench converter (I-WI-SS), and insert it into the surgical wrench (I-TWS-B45/B100).

Pick up and carefully remove the implant from the sterile vial / or fully seat the implant (Step 5)


Place the implant into the prepared osteotomy at 15-20rpm and with maximum torque set at 70Ncm



(Fig. 10)



(Fig. 11)




(Fig. 12)

STRAIGHT & CO-AXIS® IMPLANTS (FIXTURE MOUNTED)

Step 4: Implant placement (Fig. 13)

Connect the handpiece insertion tool (I-CON-IT) to the handpiece.


Engage the implant mount. Carefully remove the implant from the sterile vial. The I-CON-IT must fully engage the hex of the fixture mount.

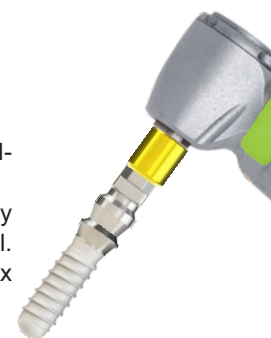

(Fig. 13)

Alternatively (Fig. 14)

Connect the handpiece insertion tool (I-CON-IT) and the wrench insert converter (I-WI-CST) to the torque wrench (I-TWS) and extract the implant from its packaging.

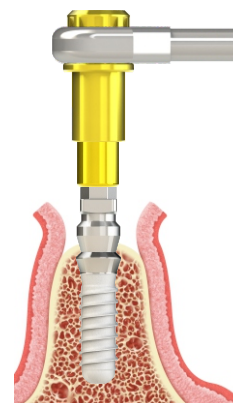


(Fig. 14)

Step 5: Fully seat the implant

To fully seat the implant follow implant placement steps as set out above. (Alternatively section points 1 and 2)

Once the implant is fully seated, loosen the fixture mount screw with the Torx Driver (I-SCS-M) and remove the fixture mount. (Fig. 15)

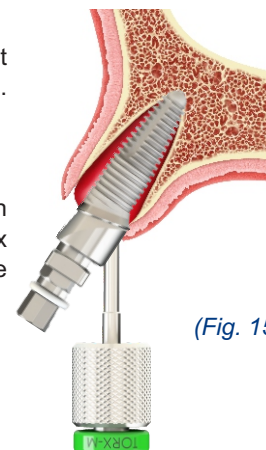

(Fig. 15)

Note:

- Use light finger force on the wrench when levelling the implant. Excessive torque (>70Ncm) with the wrench should be avoided, as this will cause too much compression in the bone or damage to the implant. A torque exceeding the maximum limit indicates that the implant should be retrieved and additional drilling should be performed in the site.
- Because the implants are self-tapping, it is recommended to stop rotation once the implant has reached the prepared depth. The implant may continue to advance beyond the drilled depth with further rotations, owing to the effective self-tapping thread. Care should be taken not to countersink the implant too far, especially in soft bone. There is also a risk that the implant may spin.

Loading times

Healing period is generally 3-4 months in the mandible and 4-6 months in the maxilla; however, healing periods may vary for each patient. When a shorter healing time or immediate loading is being considered, the assessment must be based on the individual clinical situation (i.e. bone quality, bone quantity, primary stability achieved, loading conditions, design of super-structure, etc.) Implants may be immediately temporized on single or splinted multiple-unit restorations, if good primary stability is achieved. Immediately temporized restorations should be kept out of occlusion. The patient should adhere to a soft diet and place minimal forces on the restoration for 6-12 weeks.

Troubleshooting

Implant mobility: If the fixture is very loose, consider removal and replacement with a wider diameter fixture, without further drilling.

Poor fixture alignment: If the angular misalignment is less than 30°, the problem can be addressed using angulated abutments. If the angle is greater than 30°, remove the implant and allow the surgical site to heal for approximately six months. Repeat surgery on the same area after the healing period, or use a Co-Axis® implant to take full advantage of available bone.

Exposed threads: If the implant threads are exposed in the coronal region, perform a bone augmentation procedure.

Over countersinking: Over countersinking can cause complications with primary stability in cortical bone. The countersink should not extend beyond the cortical region whenever possible. Continue with normal treatment protocol, but it is recommended to avoid immediate or early loading, and to pay special attention to the stability of the implant in the first 3-6 months after placement.

Clinical benefits

Patients can expect to have their missing teeth replaced and/ or crowns restored.

Healing

The healing time required for osseointegration depends on the individual and treatment protocol. It is the responsibility of the practitioner to decide when the implant can be restored. Good primary stability will govern if immediate loading can be done.

Implant care and maintenance

Potential implant patients should establish an adequate oral hygiene regime prior to Implant therapy. Proper post-operative, oral hygiene and implant maintenance instructions must be discussed with the patient, as this will determine the longevity and health of the Implants. The patient should maintain regular prophylaxis and evaluation appointments.

Materials

Implant: Commercially pure titanium (grade 4).

Side effects

Potential Side Effects and Temporary symptoms: Pain, swelling, phonetic difficulties, gingival inflammation. More persistent symptoms: The risks and complications with implants include, but are not limited to: (1) allergic reaction(s) to implant and/or abutment material; (2) breakage of the implant and/or abutment; (3) loosening

of the abutment screw and/or retaining screw; (4) infection requiring revision of the dental implant; (5) nerve damage that could cause permanent weakness, numbness, or pain; (6) histologic responses possibly involving macrophages and/or fibroblasts; (7) formation of fat emboli; (8) loosening of the implant requiring revision surgery; (9) perforation of the maxillary sinus; (10) perforation of the labial and lingual plates; and (11) bone loss possibly resulting in revision or removal.

Breakage

Implant and abutment fractures can occur when applied loads exceed the tensile or compressive strength of the material. Potential overloading conditions may result from; deficiencies in implant numbers, lengths and/or diameters to adequately support a restoration, excessive cantilever length, incomplete abutment seating, abutment angles greater than 30 degrees, occlusal interferences causing excessive lateral forces, patient parafunction (e.g., bruxing, clenching), loss or changes in dentition or functionality, inadequate prosthesis fit, and physical trauma. Additional treatment may be necessary when any of the above conditions are present to reduce the possibility of hardware complications or failure.

Changes in performance

It is the responsibility of the clinician to instruct the patient on all appropriate contraindications, side effects, and precautions as well as the need to seek the services of a trained dental professional if there are any changes in the performance of the implant (e.g., looseness of the prosthesis, infection or exudate around the implant, pain, or any other unusual symptoms that the patient has not been told to expect).

MR Conditional

Non-clinical testing and MRI simulations were performed to evaluate the dental implant system offered by Southern Implants. Non-clinical testing demonstrates that these products are MR Conditional. A patient with an implant from a Southern Implants System can be scanned safely in an MR system under the following conditions:

- Static magnetic field of 1.5 Tesla and 3 Tesla only
- Maximum special gradient magnetic field of 4,000 gauss/cm (40T/m)
- Maximum MR system reported whole body averaged specific absorption rate (SAR) of 2 W/kg and head average SAR of 3.2 W/kg, for 15 minutes of scanning (i.e., per pulse sequence) in the normal operating mode

The scanning conditions defined above will produce a maximum temperature increase of 4.9 °C in implants from Southern Implants systems after 15 minutes of continuous scanning (i.e., per pulse sequence).

In non-clinical testing, the image artifact caused by implants from Southern Implant System extends approximately 10 mm from this device when imaged with a gradient echo pulse sequence and a 3 Tesla MR system.

Disposal

Disposal of the device and its packaging; Follow local regulations and environmental requirements, taking different contamination levels into account. When disposing of spent items, take care of sharp drills and instruments. Sufficient PPE must be used at all times.

Disclaimer of liability

This product is part of the Southern Implants product range and should only be used with the associated original products and according to the recommendations as in the individual product catalogues. The user of this product has to study the development of the Southern Implants product range and take full responsibility for the correct indications and use of this product. Southern implants do not assume liability for damage due to incorrect use. Please note that some Southern Implants products may not be cleared or released for sale in all markets.

Notice regarding serious incidents

Any serious incident that has occurred in relation with the device must be reported to the manufacturer of the device and the competent authority in the member state in which the user and / or patient is established.

The contact information for the manufacturer of this device to report a serious incident is as follows:

sicomplaints@southernimplants.com

Basic UDI

Product	Basic-UDI Number
Basic-UDI for General Dental Implants	600954403869

Related literature & catalogues

CAT-2005 - Internal Octagon (IT) Implants Product Catalogue

Symbols and Warnings

 Manufacturer: Southern Implants 1 Albert Rd, P.O Box 605 IRENE, 0062, South Africa. Tel: +27 12 667 1046	 2797	 Prescription device*	 Sterilization using Irradiation	 Non-sterile	 Caution	 Consult instruction for use	 Use by date (mm-yy)	 Do not reuse	 Do not re-sterilize	 Batch code	 Do not use if package is damaged	 Medical Device
* Prescription device: Rx only. Caution: Federal Law restricts this device to sale by or on the order of a licenced physician or dentist.						Canada licence exemption: Please note that not all products may have been licensed in accordance with Canadian law.						
All rights reserved. Southern Implants, the Southern Implants logotype and all other trademarks used in this document are, if nothing else is stated or is evident from the context in a certain case, trademarks of Southern Implants. Product images in this document are for illustration purposes only and do not necessarily represent the product accurately to scale.												